
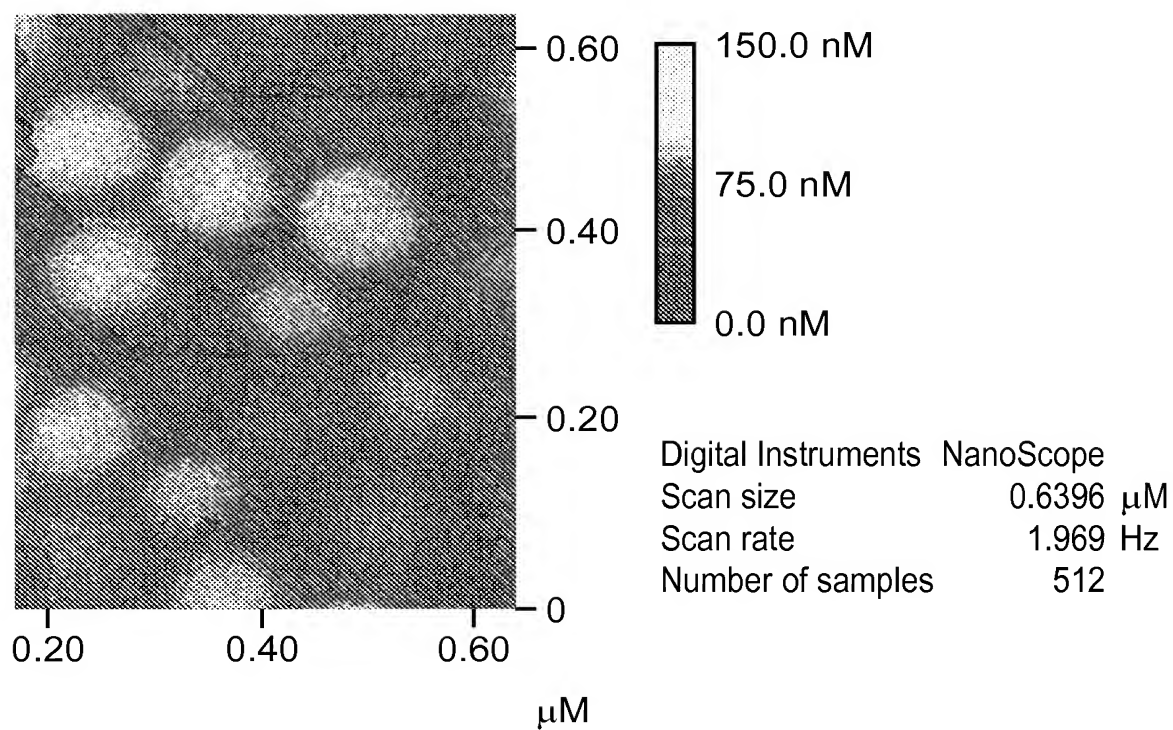


Replacement Sheet

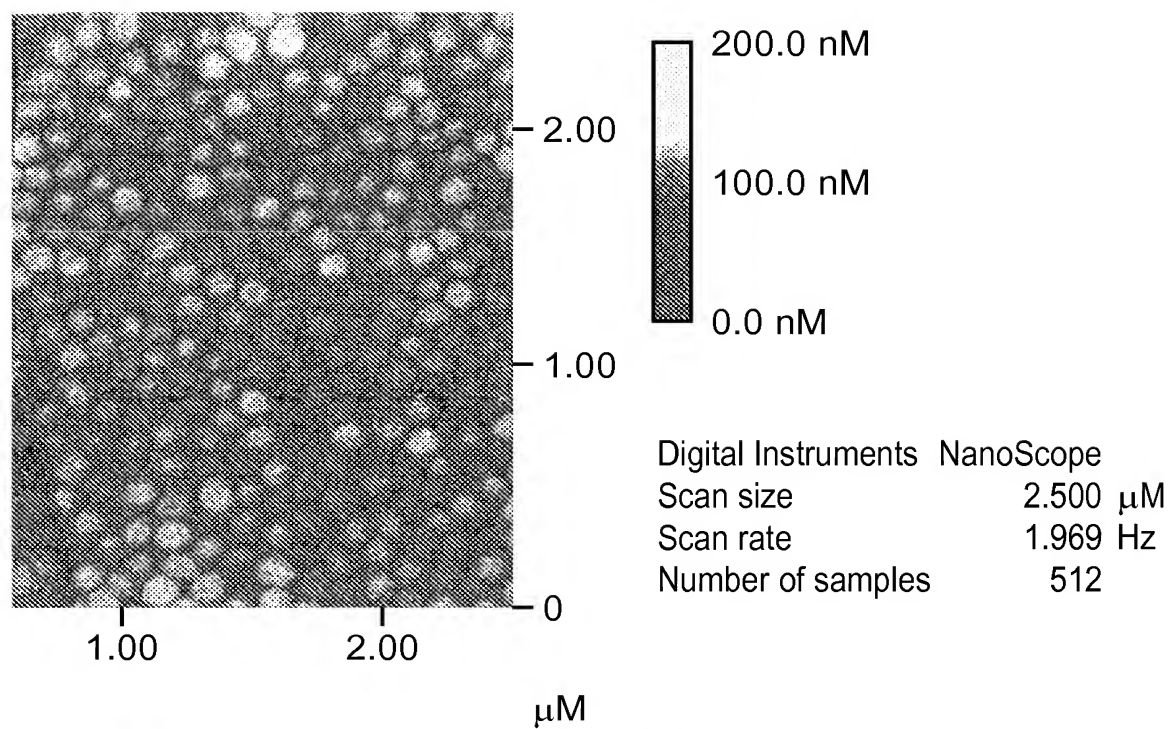

63% MMA/27% BA/3% DVB

Internally crosslinked nanoparticles ($d \approx 230 \text{ nm}$)

FIG. 1

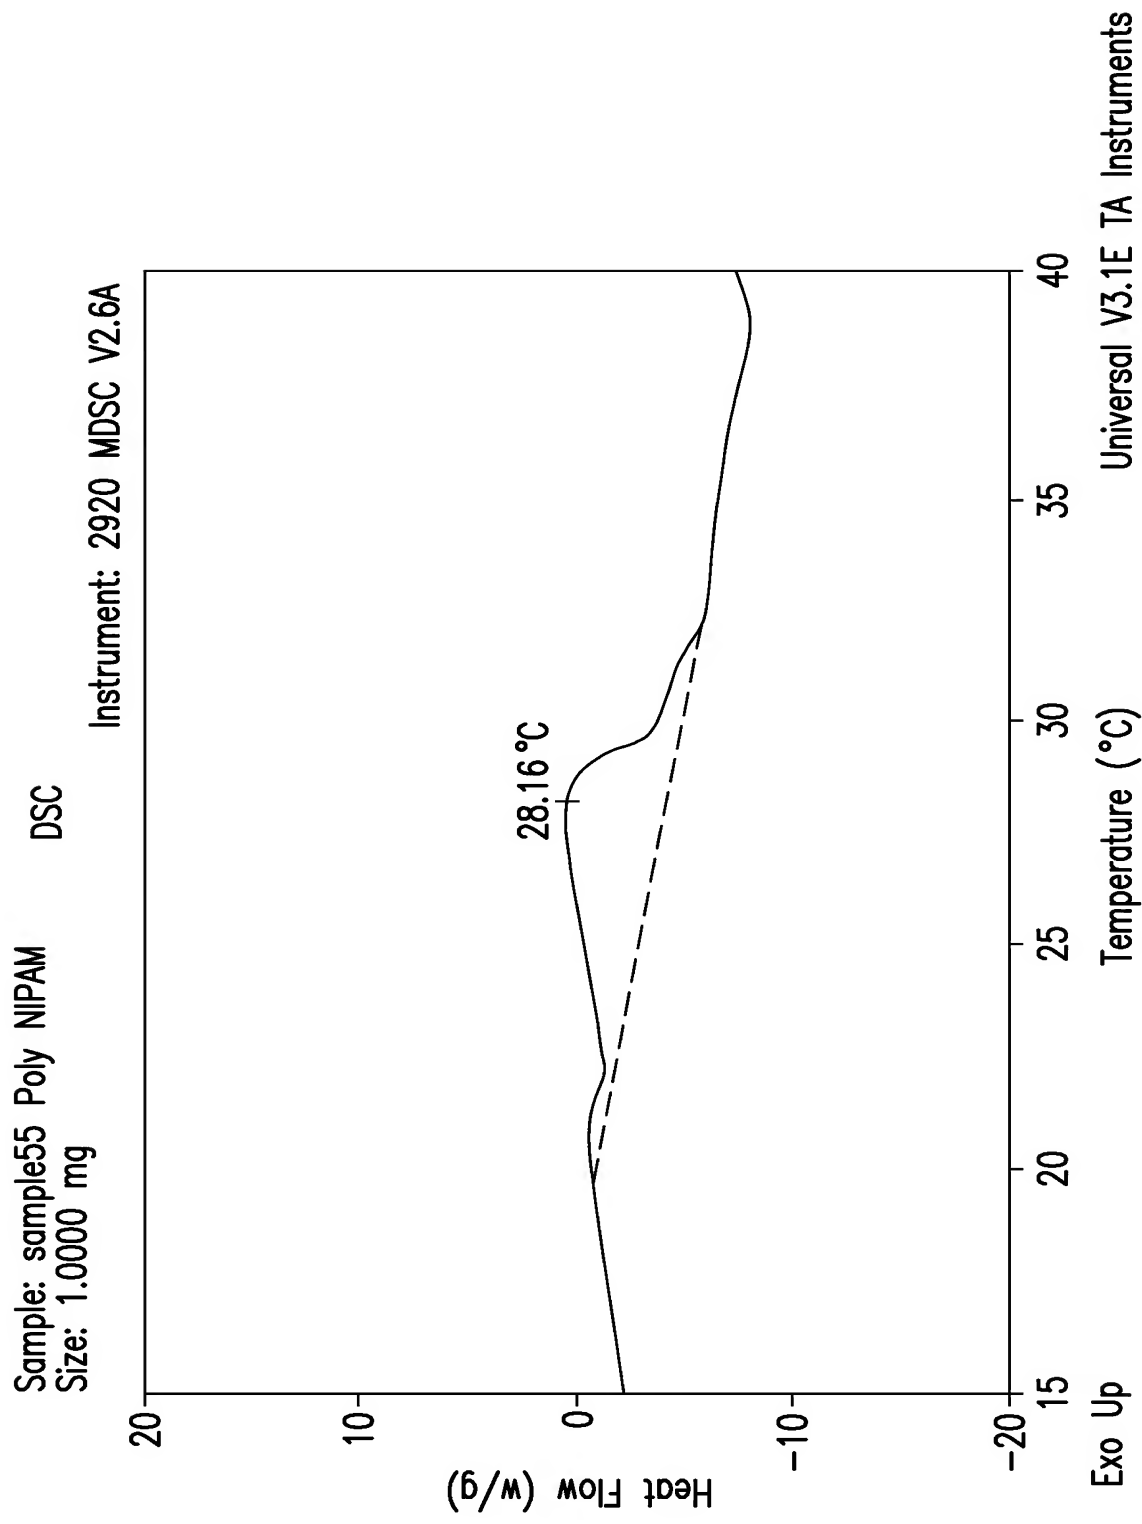



FIG.2

Sample: sample4 20%MA 80% NIPAM

Size: 1.0000 mg

DSC


Instrument: 2920 MDSC V2.6A

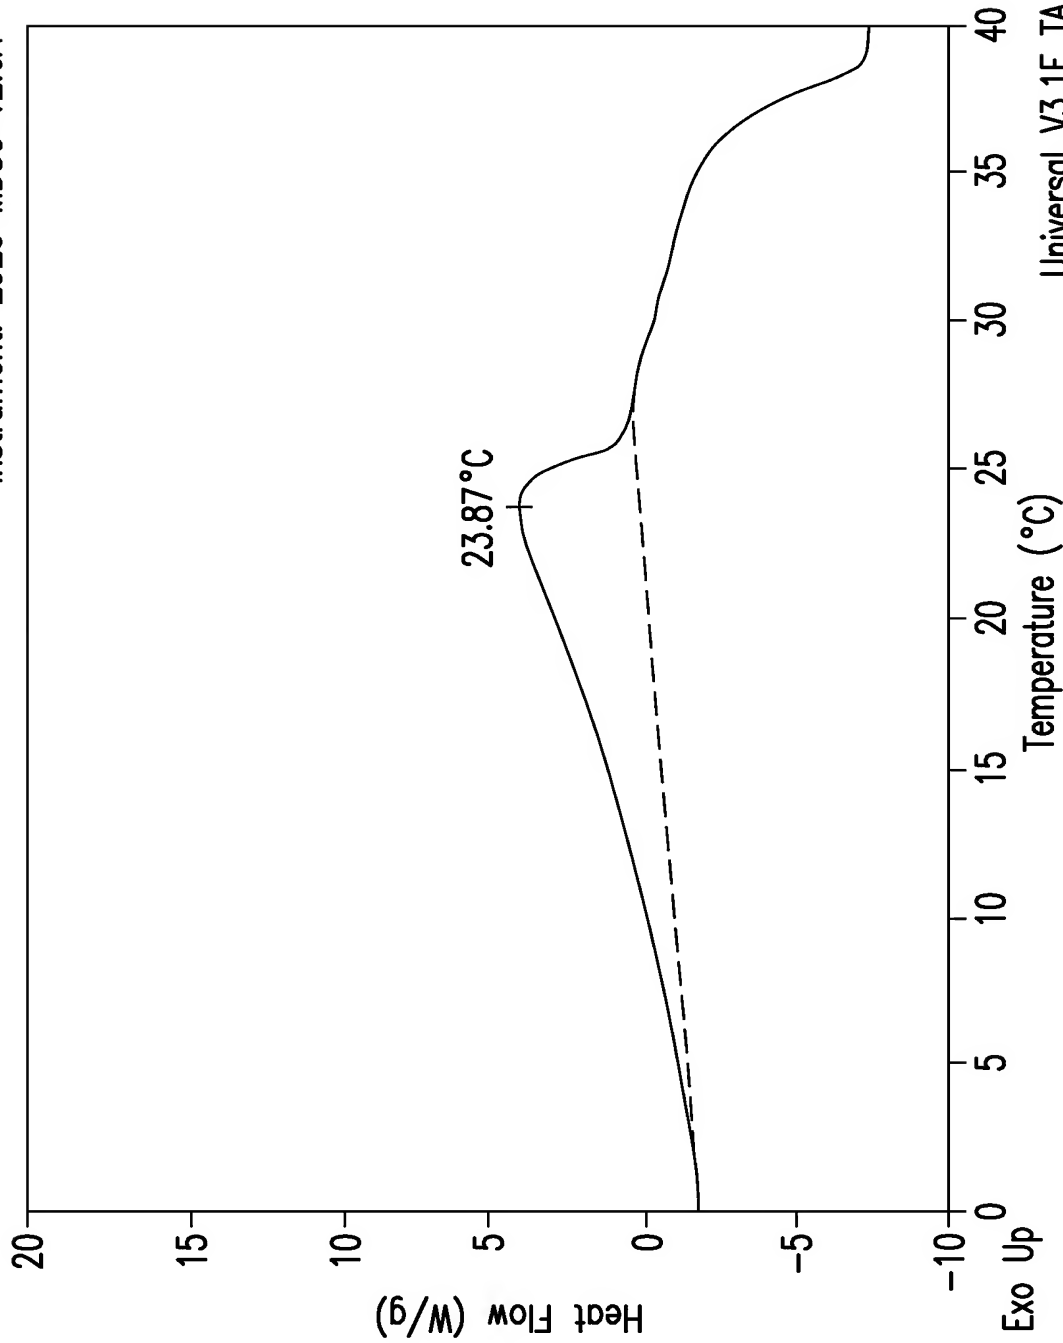

Universal V3.1E TA Instruments

FIG.3

PAM-sample 30%MA 70% NIPAM DSC Run Date: 26-Sep-03 15:54
mg Instrument: 2920 MDSC V2.6A

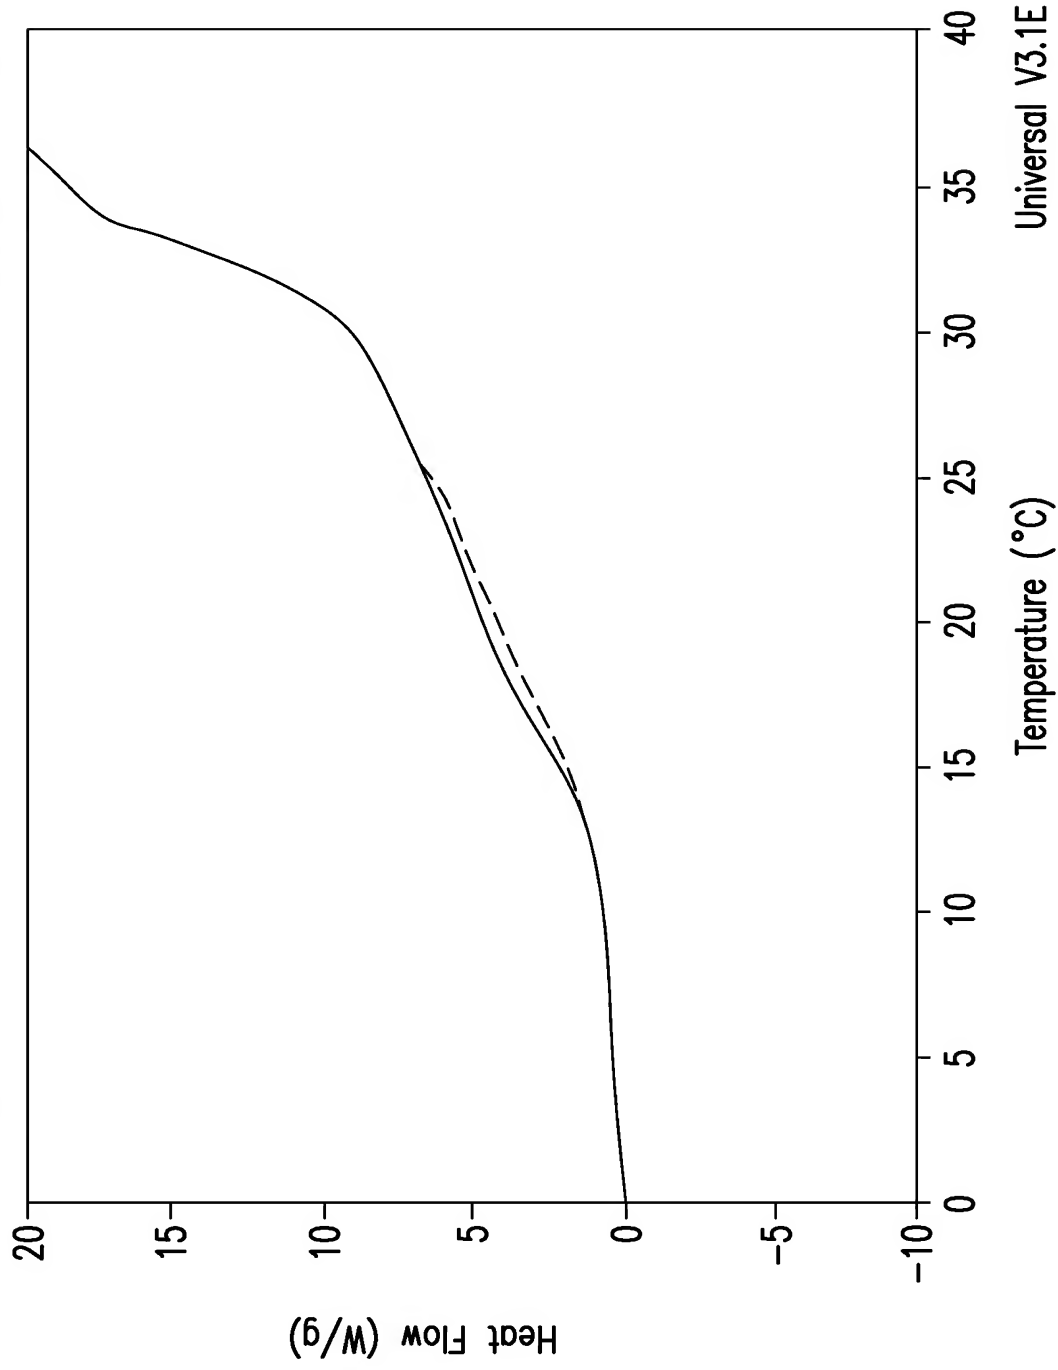

Universal V3.1E TA Instruments

FIG.4

Replacement Sheet

Sample: scott COPOLYMER 23% AN/77% NIPAM in water
 Size: 6.0000 mg
 DSC
 File: scott sample with water
 Operator: nikki
 Run Date: 1-Mar-01 13:22

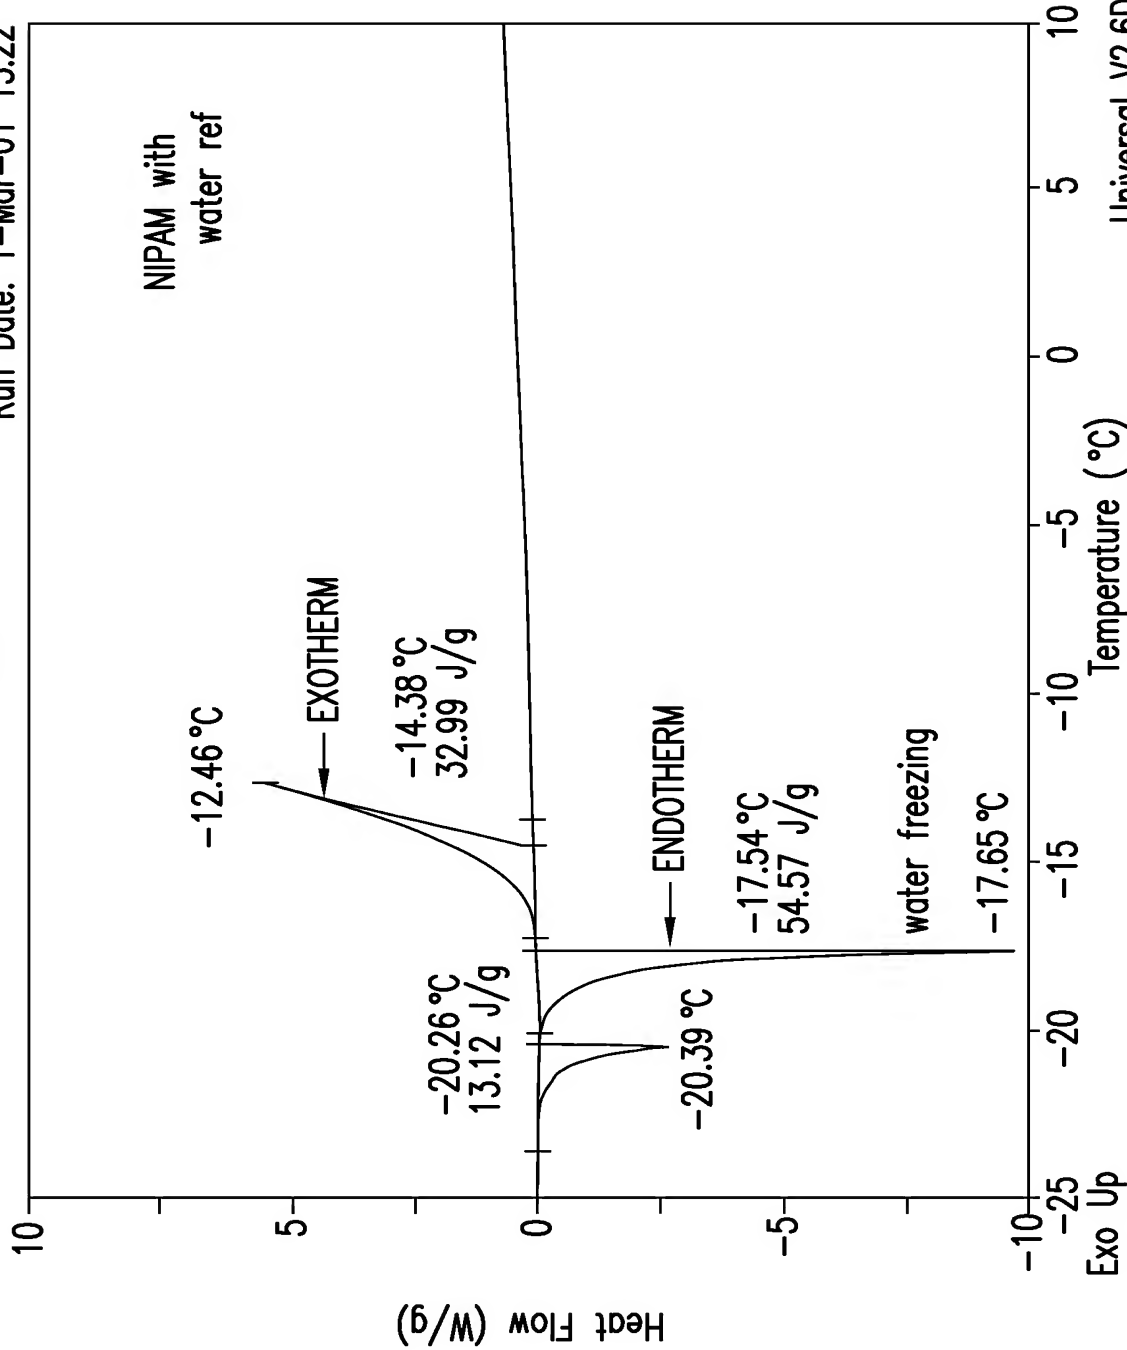


FIG.5

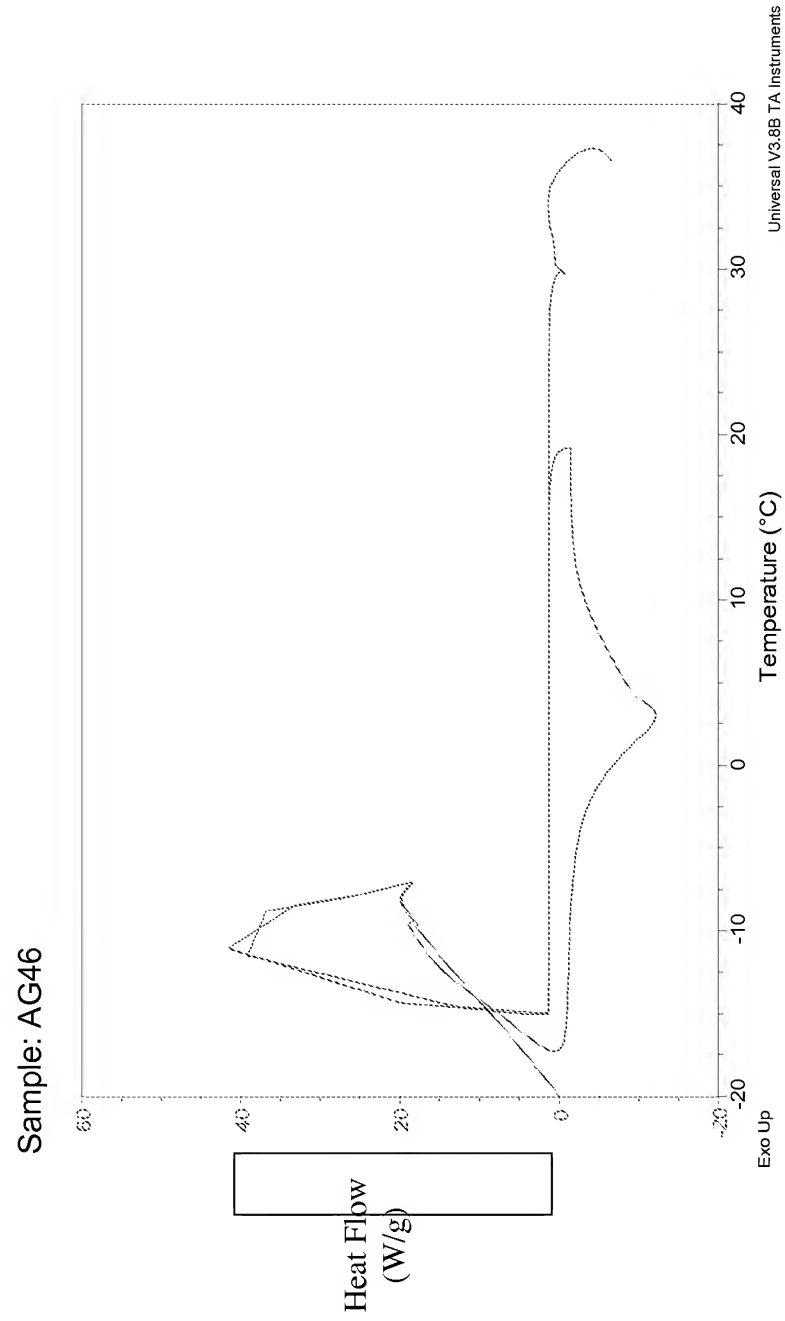


FIG. 8